


# YA015004000.rsd

(VSWR) Ref Level : 0 dB Ref Offset : 0.0 dB  
 Detector : Sample Trigger Mode : Free Run  
 Trace : Clear / Write  
 RBW : 1kHz WBW : 3 MHz  
 SWT : 1s

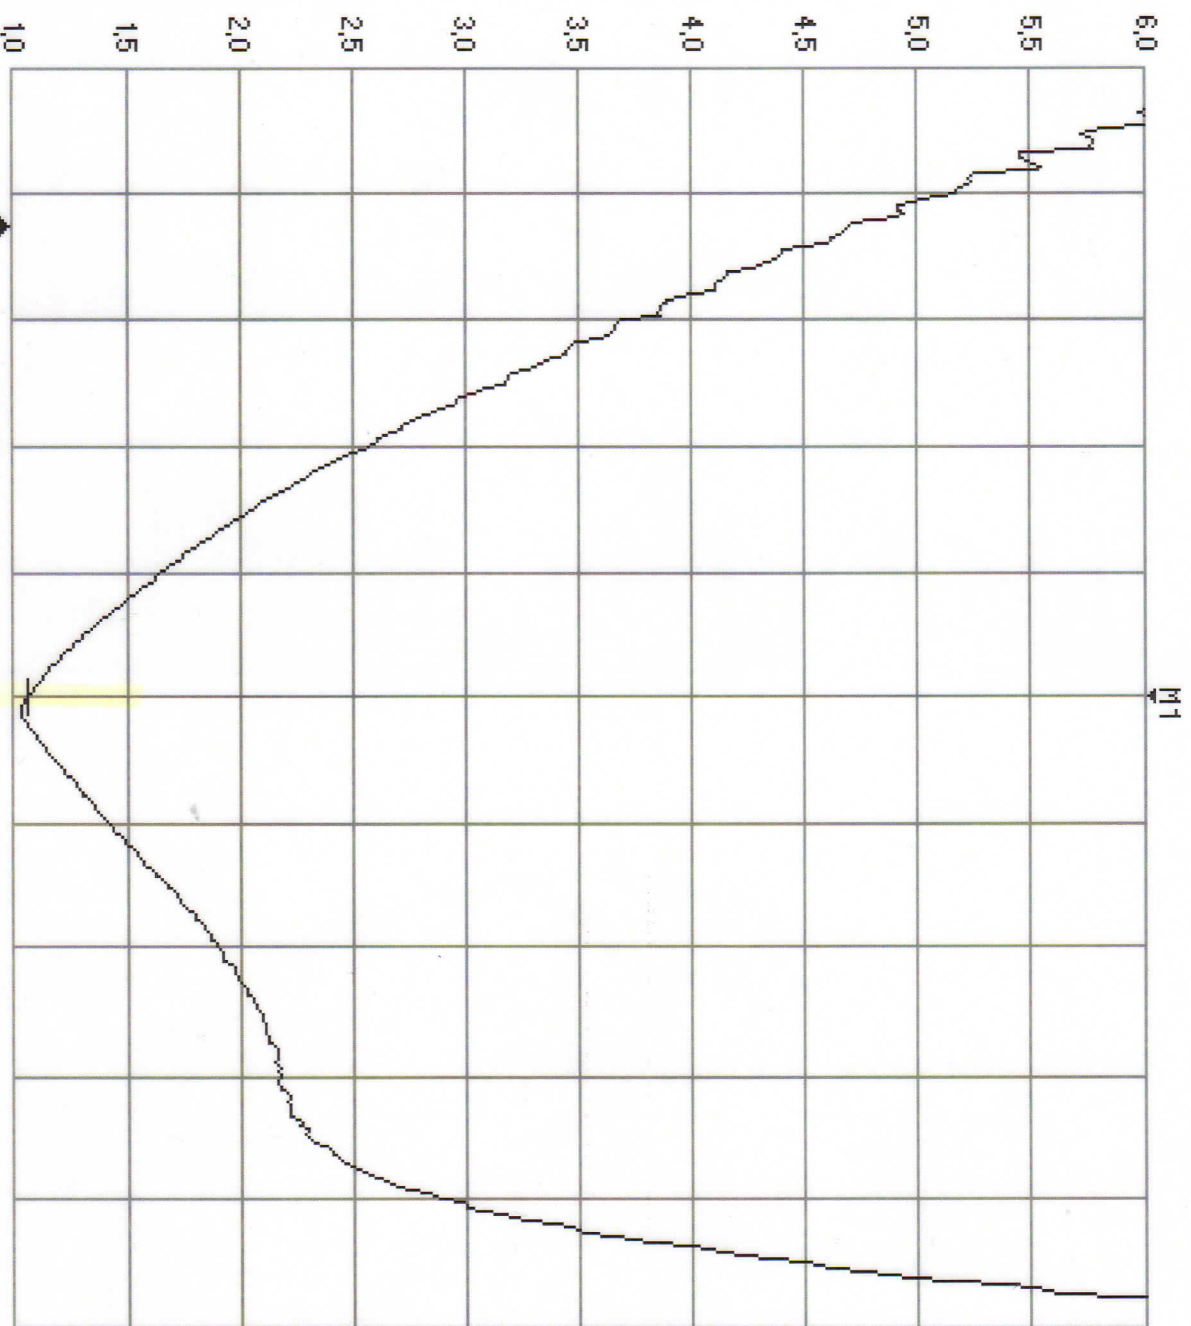

Start Frequency : 140 MHz Stop Frequency : 160 MHz  
 Center Frequency : 150 MHz Span : 20 MHz  
 Magnitude (Reflection) vector

File Name	Trace
YA015004.000	
Name	: Magnitude (Reflection)
Ref Level	: 0 dB
Range	: VSWR 1-6
BW	: Hz
Result	: .....
Averaging	: .....

Parameter	Status
VSWR-Bridge	: FSH-Z3
Center Frequency	: 150 MHz
Span	: 20 MHz
Ref Offset	: 0.0 dB
Trace Offset	: 0.0 dB
RF Attenuator	: 0 dB
Preamplifier	: Off
Dynamic Range	: Low Distortion
RF Input	: 50 Ohm
RBW	: 1 kHz
WBW	: 3 MHz
SWT	: 1 s
Trace Mode	: Clear / Write
Detector	: Sample
Trigger Mode	: Free Run
Trigger Level	: .....
Trigger Delay	: .....
Calibration Kit	: FSH CalKit
Offset Length	: 0 mm
Upper Limit	: .....
Lower Limit	: .....
External Reference	: Disabled
Date	: 25.03.2014
Time	: 13:20:05
Instrument	: FSH13 - 100888
Operator	: R. Joachims

Markers
M1 : 150 MHz : 1.0567 (VSWR)